

# **INSTRUCTION MANUAL**

Waveform Recording Program

## **VX-56WR**

 **RION CO., LTD.**

3-20-41 Higashimotomachi, Kokubunji, Tokyo 185-8533, Japan

<http://www.rion.co.jp/english/>





# Organization of This Manual

This manual describes recording functions, playback functions, and other operation principles of the Waveform Recording Program VX-56WR.

The manual consists of the chapters listed below. You should also consult the documentation for the Tri-axial Groundborne Vibration Meter VM-56.

## Outline

Gives basic information on the functions of the VX-56WR.

## Installation

Explains about installation of the VX-56WR.

## Reading the Display

Explains various items that appear on the display during recording.

## Menu Screens

Explains how to use the menus.

## Waveform Recording

Explains the steps to take for waveform recording.

## Store Data Format and File Structure

Explains the format of stored data and how the files are organized.

## Card Capacity and Recording Time

Explains the relationship between rated memory card capacity and recording time.

## Communication Commands

Explains additional commands that become available when the waveform recording function is loaded.

## Reanalysis with AS-70GV

Explains reanalysis with AS-70GV.

## Specifications

Lists the technical specifications of the VX-56WR.

\* All company names and product names mentioned in this manual are trademarks or registered trademarks of their respective owners.

# Software Usage License Agreement

Important
<p><b>In order to use this Software, you must agree to the terms of the Software Usage License Agreement (hereinafter “this Agreement”). Please read the following text carefully, and only proceed to use the Software if you agree to be bound by all the terms and conditions of this Agreement.</b></p>

## Article 1 Authorized Use

This Software (including updated or customized versions) is designed for use with the Tri-axial Groundborne Vibration Meter VM-56 (hereinafter “the Product”). You are authorized to use the Software only in conjunction with the Product, in such a way as stipulated in this Agreement.

## Article 2 Ownership of the Software

All rights to this Software are retained by Rion Co., LTD, (hereinafter “Rion”) and/or its rightful owners. This Agreement grants you only a limited right to use the Software. This Agreement does not grant you any other rights other than specified herein.

## Article 3 Limitations to Use and Transfer

1. This Agreement does not grant you any rights to copy the Software and any associated documentation.
2. This Agreement does not grant you any rights to alter or modify the Software.
3. This Agreement does not grant you any rights to reverse engineer, de-compile, recompile, or disassemble the Software.
4. Unless prior written permission from Rion has been obtained, this Agreement does not grant you any rights to lend the Software to any third parties, regardless of whether this is done for payment or free of charge.
5. This Agreement does not grant you any rights to transfer the rights specified in this Agreement to any third parties.

## Article 4 Warranty Scope

1. Rion does not make any representation or promise that this Software will be able to perform without problems under any and all conditions. If a problem occurs while the Software is being used under normal conditions, contact Rion using the information provided in the Instruction Manual. As far as possible based on the information provided by you about the problem, Rion will provide guidance and information about possible errors, improved operation procedures and similar.
2. Rion (including any affiliated companies and subsidiaries) assumes no liability for any damages caused by alteration or loss of data stored in the Product which is attributable to a problem with the Software.
3. In no event does Rion assume liability for any kind of direct or indirect damage, loss of profit or anticipated gain, or any other damage caused by the use of the Software, or the inability to use the Software.
4. In no event does Rion assume liability for any problem caused by an alteration or modification of the Software by you. Rion also does not assume liability for any damage caused to yourself by such an alteration or modification.
5. Liability of Rion for any damages will not exceed the actual price that was paid for the license to use the Software. This limitation does not apply in the case of intentional faults or gross negligence.

## Article 5 Remedy

1. Rion guarantees that the Software as supplied contains the functions that are explicitly listed in the specifications.
2. If the software does not operate according to specifications, and the cause is the responsibility of Rion, and if this is detected and Rion is informed of this fact within 90 days from the purchase date of the Software, Rion will undertake to remedy the problem free of charge.
3. In cases other than above, Rion will undertake to remedy the problem against charge.

## **Article 6 Duration of this Agreement**

1. You can terminate this Agreement at any time by stopping to use the Software and destroying the Software and all associated documentation.
2. If you violate any of the conditions of this Agreement, Rion can cancel this Agreement and terminate the usage of the Software. In such a case, you are obligated to destroy the Software and all associated documentation (including any unauthorized copies).

## **Article 7 Other Items**



If the Software and the Product are taken from Japan to any other country, the Japanese Foreign Exchange and Foreign Trade Law, the United States Export Administration Act, and all other applicable laws and regulations must be strictly observed. This Agreement shall be exclusively governed by the laws of Japan.

## **Article 8 Third Party Beneficiaries**

This Software includes components for which the rights are held by other parties except Rion. In the case of a violation of this Agreement, in addition to Rion, such third parties shall also have the right to demand compensation for damages.

# FOR SAFETY

In this manual, important safety instructions are specially marked as shown below. To prevent the risk of severe damage to the program or peripheral equipment, make sure that all instructions are fully understood and observed.

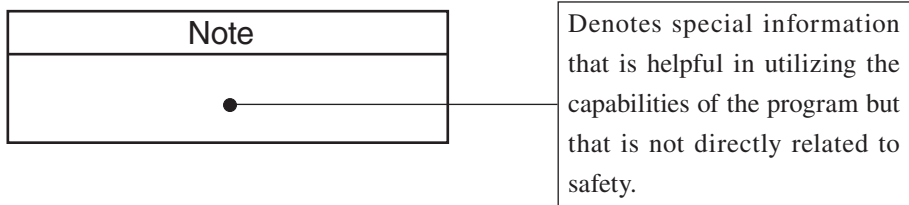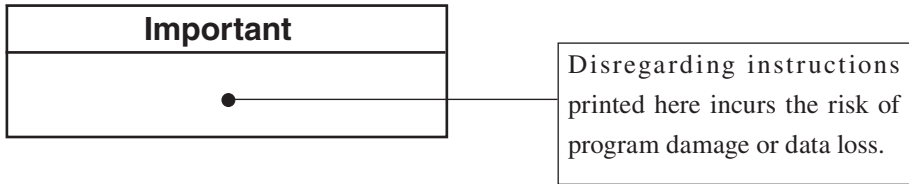

# Contents

Software Usage License Agreement .....	ii
FOR SAFETY .....	v
Outline .....	1
Installation .....	2
Reading the Display .....	3
Recording screen .....	3
Menu screen .....	4
Menu Screens.....	5
Waveform Recording.....	8
Total recording .....	9
Analysis of recorded files.....	11
Store Data Format and File Structure .....	12
Card Capacity and Recording Time .....	14
About card capacity and recording time.....	14
Communication Commands .....	16
List of commands .....	16
Command Description .....	17
Reanalysis with AS-70GV .....	19
Specifications .....	20



# Outline

The waveform recording program VX-56WR is an option program for adding acceleration waveform recording function to the Tri-axial Groundborne Vibration Meter VM-56 main unit. Acceleration waveform is saved in WAVE format, and recording starts at the same time as measurement. Combined use with waveform analysis software enables 1/3 octave band analysis.

As an outline of the function, the signal input from the acceleration pickup is recorded at a sampling frequency of 2 kHz. Also, it is possible to record the calibration signal output from the VM-56 by switching the input signal. Recording is also started at the same time that the manual store or auto store of the main unit is started, and the recording is also ended at the same time that the store ends.

<b>Important</b>
Use SD memory cards provided by Rion. The performance of other cards is not guaranteed.

# Installation

Follow the procedure described in the separate “Optional program installation / uninstallation” to install the VX-56WR program in the VM-56 unit.


<b>Important</b>
Never format the optional program card with SD memory card formatting software (such as SD Formatter etc.). Otherwise the program data on the card will be erased and the respective functions can no longer be used. Restoration of the erased program is not warranted.
Upgrade the firmware of the VM-56 to the latest version before installing the optional program. The latest version firmware can be downloaded from “Software downloads” of Support Room on our web site ( <a href="http://www.rion.co.jp/english/">http://www.rion.co.jp/english/</a> ).

# Reading the Display

## Recording screen

An illustration of recording screen is shown below.

(The size and font of the actual display may differ.)

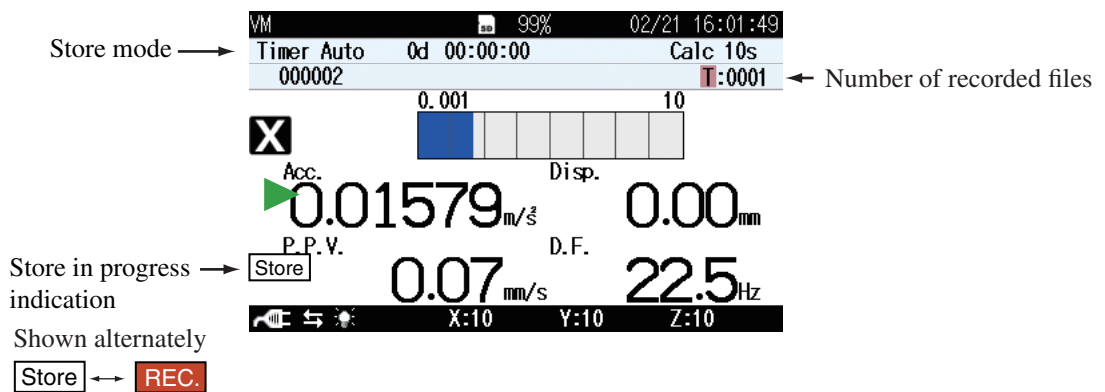

### Store mode

Shows the selected mode for storing data in memory.

### Store in progress indication

Shows the store condition.

### Number of recorded files

Shows the recorded file count.

## Menu screen

The menu screen looks as follows.

MENU	Wave recording (WR) 05/11 10:09:46
Wave Rec Mode	ON(Total)
Bit Length	16bit
Wave Splitting Interval	10min
Input signal	Sensor

The screenshot shows the Wave recording (WR) screen with a light blue background. At the top right, it displays 'T:0000' with a left-pointing arrow. Below this, there are two main options: 'Measure' with a right-pointing arrow and a green play button icon, and 'Back' with a right-pointing arrow and a green double vertical bar icon. At the bottom left, there is a black bar with a white microphone icon and a left-pointing arrow. To the right of the screenshot, a text box explains that 'T' stands for total recording and '0001' is the recorded file count.

Wave recording (WR) screen

The recorded file count starts at ST0001.WAV and will stop at the maximum of ST9999.WAV.

The number shows the sequential number for the file.

A "0000" file is not created.

Note
The performance about the file after the 10,000th will not be guaranteed.

# Menu Screens



Pressing the MENU/ENTER key brings up the menu list screen. Use the  $\Delta / \nabla / \triangleleft / \triangleright$  keys to select [WR] and press the MENU/ENTER key. The wave recording (WR) screen appears. The recording condition is set on this screen. Each item of the wave recording screen is selected using the  $\Delta / \nabla$  key.

Pressing the DISPLAY key displays explanation screen of the item that has been selected.

Pressing the PAUSE/CONT key switches back to the menu list screen.

Pressing the START/STOP key switches back to the measurement screen.


As for the wave recording screen, the displayed set item is different depending on the set recording mode.

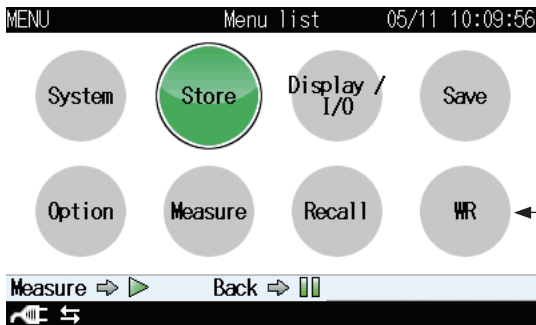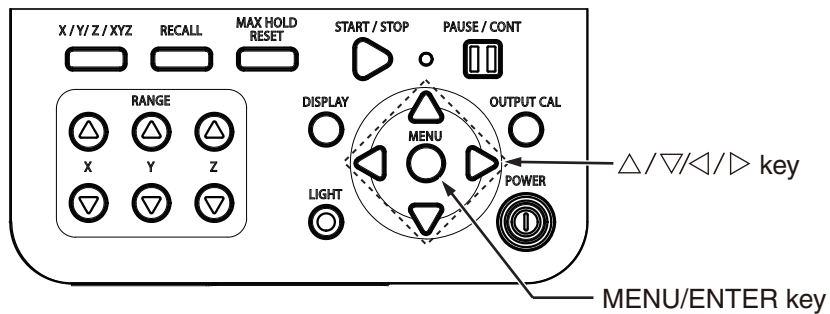

Pressing the  $\Delta / \nabla / \triangleleft / \triangleright$  keys to select [WR] and pressing MENU/ENTER key brings up the [Wave recording (WR)] screen.

Menu list screen

MENU Wave recording (WR) 05/11 10:09:46	
Wave Rec Mode	ON(Total)
Bit Length	16bit
Wave Splitting Interval	10min
Input signal	Sensor



Wave recording (WR) screen

## Wave Rec Mode

Set the waveform recording mode.

Select [Wave Rec Mode] and press the MENU/ENTER key. The Wave Rec Mode screen appears. Select the recording mode (OFF, ON (Total)) and press the MENU/ENTER key.

If “ON (Total)” is selected, all waveform are recorded from start to finish. When [Wave Rec Mode] is set to “OFF”, waveform recording will not be carried out.

## Bit Length

Select the recording data bit length. Increased accuracy of analysis can be obtained as the value increases.

Select [Bit Length] and press the MENU/ENTER key. The Bit Length screen appears. Select the bit length (16bit, 24bit) and press the MENU/ENTER key.

## Wave Splitting Interval

Select the size of one file for the entire recording.

Select [Wave Splitting Interval] and press the MENU/ENTER key. The Wave Splitting Interval screen appears. Select the splitting interval (10min, 1h) and press the MENU/ENTER key.

## Input signal

Select the signal to be input.

Select [Input signal] and press the MENU/ENTER key. The input signal selection screen appears. Select either [Sensor] or [Cal signal] and press the MENU/ENTER key. If [Cal signal] is selected, the waveform of the calibration signal will be recorded. Normally, you should select [Sensor]. When recording waveform information for the sensor signal, the setting is Fixed acceleration waveform from 0.5 Hz to sensor depending.

## Menu list

Wave Rec Mode -----	OFF, ON (Total)
Bit Length -----	16bit, 24bit
Wave Splitting Interval -----	10min, 1h
Input signal -----	Sensor, Cal signal

# Waveform Recording

The VX-56WR provides the Total (total recording) mode.

The Total mode can be used when Auto store (Auto and Timer Auto) or Manual store (Manual) is selected.

Select the appropriate recording function before starting to record.

Verify that an SD memory card with sufficient free space is inserted in the card slot of the VM-56. If no card is inserted, recording cannot be carried out.

For information on how to access and use the setup screen and menus, see the section “Menu Screens”.

The recorded waveform data is saved as the following channel to the WAVE file.

X axis direction: channel 1

Y axis direction: channel 2

Z axis direction: channel 3


Note
After installation is complete, the SD card from which the VX-56WR program was installed can be used as a memory card for storing data.
Prior to measurement, it is recommended first to format the memory card for storing data with this unit.



## Total recording

1. Select measurement parameters as described in the “Manual”, “Auto”, and “Timer Auto” sections of the “Store Operation” in the documentation (Instruction Manual) of the VM-56.
2. Access the waveform recording menu screen, set [Wave Rec Mode] to “ON (Total)”, and make appropriate settings for [Bit Length] and [Wave Splitting Interval].

MENU		Wave recording (WR) 05/11 10:09:46	
Wave Rec Mode	ON(Total)	←	Total
Bit Length	16bit	←	16bit, 24bit
Wave Splitting Interval	10min	←	10min, 1h
Input signal	Sensor	←	Sensor, Cal signal



Wave recording screen  
(Wave Rec Mode: ON (Total))

3. Press the START/STOP key to return to the measurement screen.
4. Store
  - 4-A. Manual store
 

Press the START/STOP key to start measurement, and press the START/STOP key again to stop.

To save the measured data and recorded data, select “Store data” on the data save confirmation screen when the measurement is stopped.

During a recording session, the PAUSE/CONT key (PAUSE function) can be used.
  - 4-B. Auto, Timer Auto store
 

When you press the START/STOP key to start auto store, recording also starts simultaneously.

Files are created and saved for each recording period.

To stop recording, press the START/STOP key.


During Auto store, the PAUSE/CONT key (PAUSE function) cannot be used.

The graphs below show the operation principle of total recording.


“Measurement finished” is displayed after measurement is completed. When saving, select “Save data” and push “MENU” key.

“Measurement finished” is displayed after measurement is completed. To save, select “Save data” and push “MENU” key.

#### Total recording (with manual store)

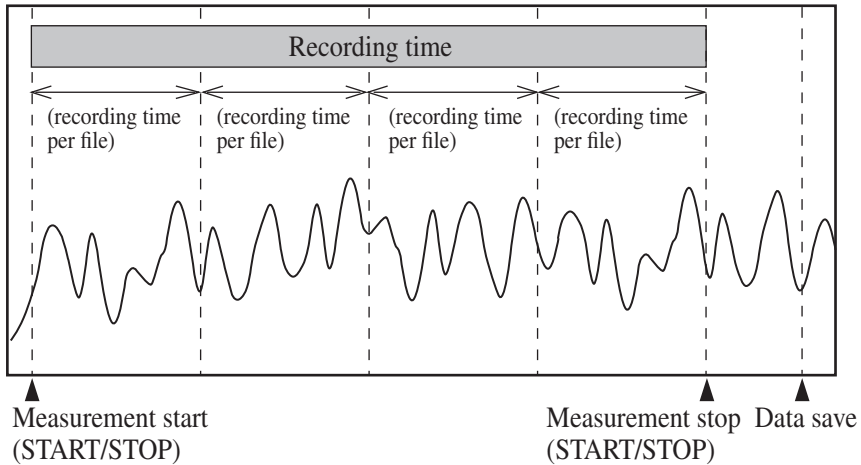

#### Total recording (with auto store)

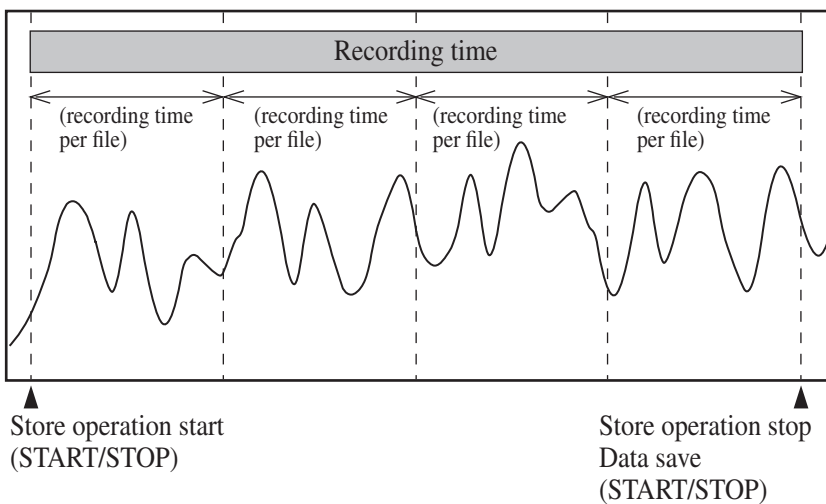

## **Analysis of recorded files**

Recorded files can be analyzed with the Waveform Analysis Software AS-70GV from Rion.

Analysis of recorded information on the VM-56 is not possible.

# Store Data Format and File Structure

Folders that are used for saving data differ, depending on the selected store mode.

## Store destination folder

Files are saved in the sub folder WAVE which is created in the store folder specified by store name.

Example: Manual\_0123/WAVE (with manual store)

Auto\_0123/WAVE (with auto and timer auto store)

## File name of recording data

Recording files are named as shown below.

VM\_001\_20180701\_123456\_0123\_0001\_ST0001.wav

The diagram shows the file name VM\_001\_20180701\_123456\_0123\_0001\_ST0001.wav with brackets and lines indicating the following components:

- Index number: 001
- Date of recording start: 20180701
- Recording start time: 123456
- Store name: 0123
- Address: 0001
- Recording mode: ST0001

Store name: 0000 to 9999

Address: 0000 to 9999 (Auto store is fixed to 0000)


Recording mode: Shown as ST (indicating total recording) followed by the sequential file number

### Note

The performance about the file after the 10,000th will not be guaranteed.

When a file with the same name exists in the same directory, it will always be overwritten.

A sample configuration is shown below.

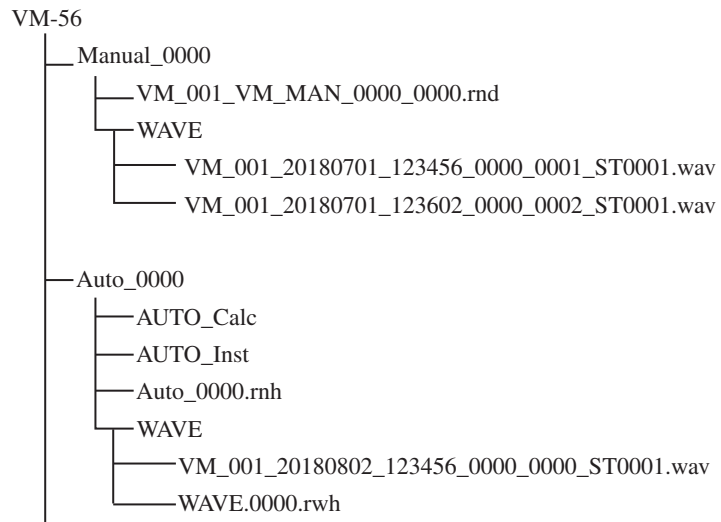

# Card Capacity and Recording Time


## About card capacity and recording time

When saving data on the SD memory card, there are two kinds of storage areas: an area for “recording data (WAVE files) + store data”, and an area dedicated to store data only.

When the area for “recording data + store data” becomes full, recording will stop, but only store data will continue to be saved in the area dedicated to store data.

If the capacity of the SD memory card is less than 2 GB, recording will always stop when the remaining capacity reaches 100 MB. After that, only store data will be saved. On SD memory cards with a capacity of 2 GB and above, recording will stop when the remaining capacity reaches 200 MB. After that, only store data will be saved.

The actual size of both store data files and recording files depends on various factors, such as store mode, bit length, and etc. When there are multiple recording data with short recording times, storage space will be wasted and the available time for recording may be up to 20 percent shorter.

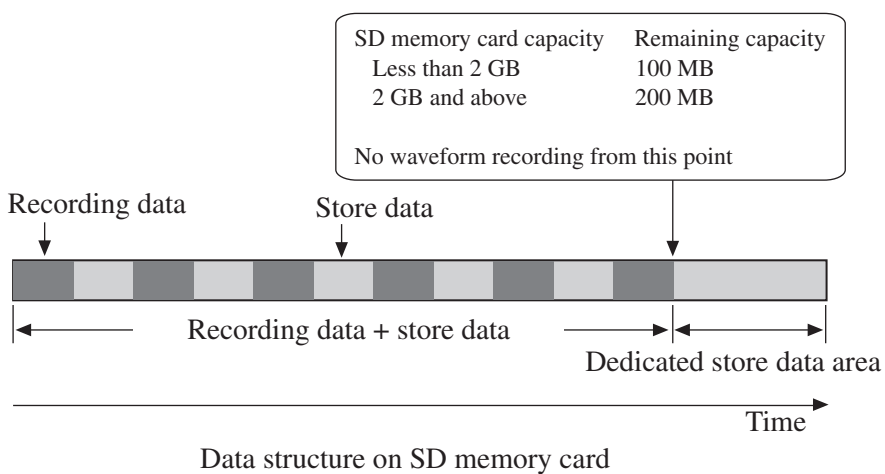

## Approximate recording times for SD memory cards

		SD memory card capacity		
		512 MB	2 GB	32 GB
Bit length	16 bit	Approx. 8 hours	Approx. 32 hours	Approx. 698 hours
	24 bit	Approx. 5 hours	Approx. 22 hours	Approx. 394 hours

Data apply for Auto store, Auto store inst 100 ms

The duration of recording with 24 bit becomes shorter than that with 16 bit because the data volume of 24 bit is about 1.5 times more.

<b>Important</b>
Use SD memory cards with a capacity of 512 MB and above.

# Communication Commands

This section lists commands that are added to the Tri-axial Groundborne Vibration Meter VM-56 when the waveform recording function is installed. For information on other commands, please refer to the instruction manual of the VM-56.

## List of commands

S: Setting command (for making settings)

R: Request command (for obtaining information on status and measurement results)

Command	Function	See page
Wave Rec Mode	Waveform recording mode (S/R) ....	17
Wave Bit Length	Bit length (S/R).....	17
Wave Splitting Interval	File split period (S/R).....	18



## Command Description

### Wave Rec Mode

#### Waveform recording mode

Setting waveform recording mode

Setting command	Wave _ Rec _ Mode, p1
Parameter	p1= "Off" p1= "Total"
Request command	Wave _ Rec _ Mode?
Response data	d1
Returned value	Same as for setting command

### Wave Bit Length

#### Bit length

Setting bit length

Setting command	Wave _ Bit _ Length, p1
Parameter	p1= "16bit" p1= "24bit"
Request command	Wave _ Bit _ Length?
Response data	d1
Returned value	Same as for setting command

## Wave Splitting Interval

### File split period

#### Setting file split period

Setting command Wave \_ Splitting \_ Interval, p1

Parameter p1= "10m"

p1= "1h"

Request command Wave \_ Splitting \_ Interval?

Response data d1

Returned value Same as for setting command


# Reanalysis with AS-70GV

When performing waveform recording with the VX-56WR, start the recording so that the recorded period is a few seconds longer than required. During analysis of the recorded WAV file with AS-70GV etc., the MTVV can only be obtained after the first second has elapsed. The transient response of the filter also has a certain influence, therefore data from a point before the specified period are required for signal processing.

## Note

To calculate the MTVV, the VM-56 uses data from one second before the current point. Therefore data from the past one second before the measurement start are required for the first one-second period.


With the VX-56WR, WAV file recording begins from the measurement start point. Therefore MTVV results may differ from the VM-56.

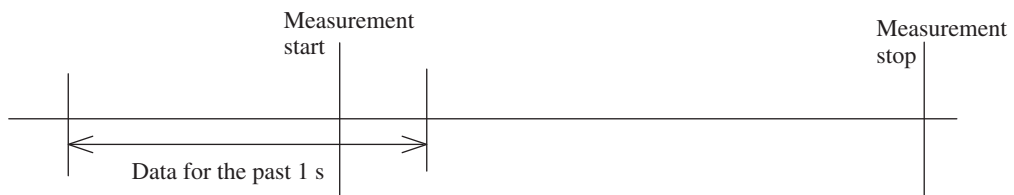

# Specifications

Compatible model	Tri-axial Groundborne Vibration Meter VM-56
Media	SD memory card      2 GB
Sampling frequencies	2 kHz
Bit length	24 bit, 16 bit
Data format	WAVE
Frequency weighting	Lower limit 0.5 Hz, Upper limit Sensor dependent
Signal-noise ratio	80 dB and over
Recording functions	
Total recording	Record all time domain waveform during auto store In manual store mode, measurement followed by store operation records the time domain waveform for the entire period of measurement
Parameter settings	
File split interval	10 minutes, 1 hour
Number of recorded data	
Auto store	9999 using a single store name
Manual store	144 per address
Battery life	Battery life will be approx. 25% shorter when waveform recording function is used
Dimensions	32 mm (H) × 24 mm (W) × 2.1 mm (D)
Weight	Approx. 5 g
Supplied accessories	
Inspection certificate	1



 This product is environment-friendly. It does not include toxic chemicals on our policy.

No. 63440 18-06